

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington 98005 USA
Phone: (425) 643 - 9866 Fax: (425) 643 - 9954 Internet: seabird@seabird.com

SENSOR SERIAL NUMBER = 1335
CALIBRATION DATE: 30-Apr-02s

CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHJ COEFFICIENTS

g = -4.15977511e+00
h = 5.25735587e-01
i = -4.61412929e-05
j = 3.47583805e-05
CPcor = -9.57e-08 (nominal)
CTcor = 3.25e-06 (nominal)

ABCDM COEFFICIENTS

a = 3.19042512e-05
b = 5.25535320e-01
c = -4.15888981e+00
d = -7.84547501e-05
m = 4.0
CPcor = -9.57e-08 (nominal)


BATH TEMP (ITS-90 °C)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.81249	-0.00000	-0.00000
-1.4008	35.0495	2.78752	7.79304	2.78754	0.00002
0.9992	35.0499	2.99395	8.03925	2.99394	-0.00001
14.9992	35.0502	4.29718	9.44459	4.29716	-0.00002
18.4992	35.0498	4.64590	9.78586	4.64590	0.00000
28.9992	35.0470	5.73574	10.78144	5.73578	0.00004
32.4992	35.0407	6.11059	11.10265	6.11056	-0.00003

Conductivity = $(g + hf^2 + if^3 + jf^4) / [10(1 + \delta t + \epsilon p)]$ Siemens/meter

Conductivity = $(af^m + bf^{2m} + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature [deg C]; p = pressure [decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

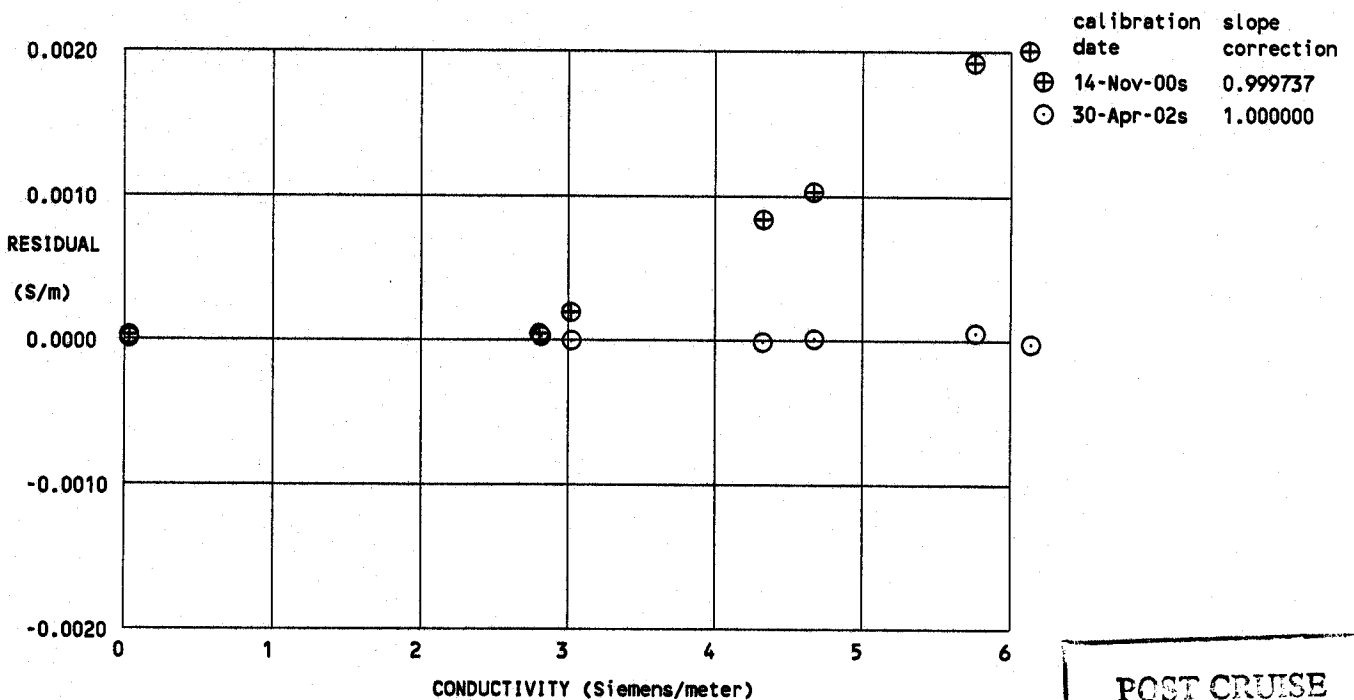

POST CRUISE
CALIBRATION