

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0154  
CALIBRATION DATE: 08-Jul-04p

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS

Soc = 0.4612

Boc = 0.0000

Voffset = -0.5156

TCor = 0.0009

PCor = 1.350e-04

BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.65	25.00	0.01	1.119	1.64	-0.00
2.09	5.00	0.00	1.022	2.09	0.00
2.37	25.00	0.01	1.386	2.37	-0.00
2.81	5.00	0.00	1.194	2.81	0.00
3.14	25.00	0.01	1.667	3.14	-0.00
3.64	5.00	0.00	1.395	3.64	-0.00
5.00	25.00	0.01	2.353	5.00	0.00
5.55	5.00	0.00	1.857	5.55	-0.00
6.46	25.00	0.01	2.886	6.46	-0.00
7.13	5.00	0.00	2.240	7.13	0.00

oxygen (ml/l) = (Soc \* (V + Voffset)) \* exp(Tcor \* T) \* Oxsat(T,S) \* exp(PCor \* P)


V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU]

Oxsat(T,S) = oxygen saturation [ml/l], P = pressure [dbar]

Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

● 08-Jul-04p -0.00

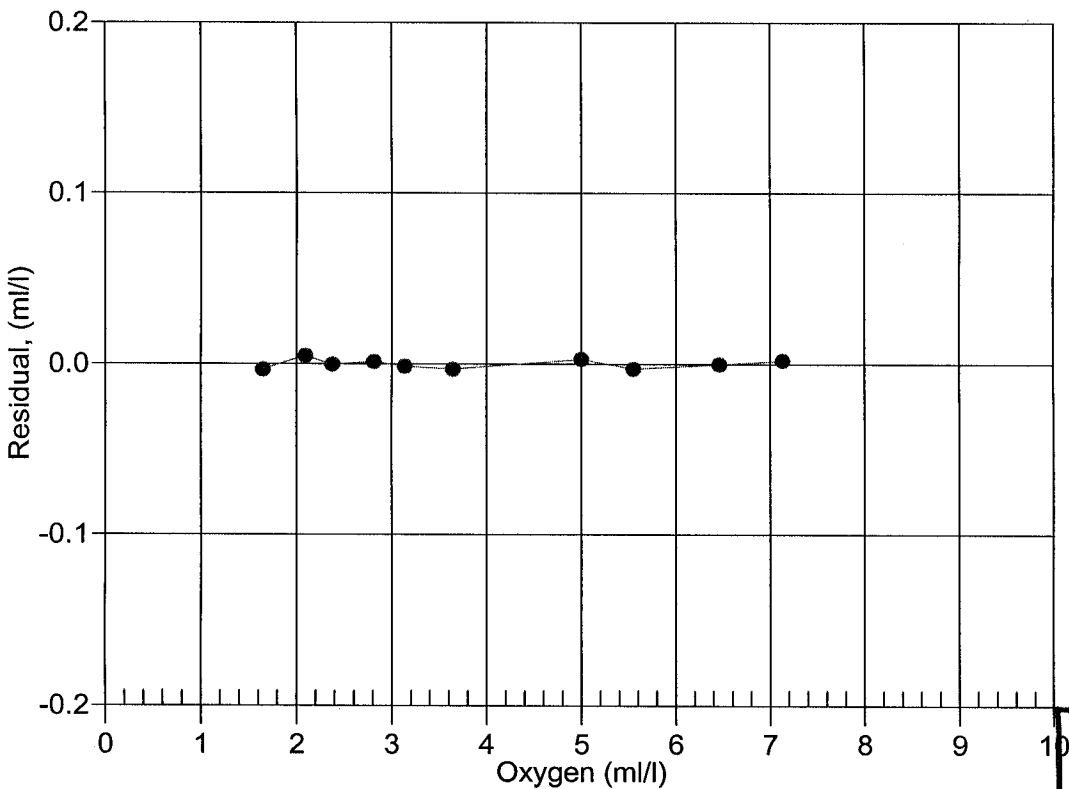

CALIBRATION  
AFTER  
MODIFICATIONS