



Phone: (425) 643-9866 Fax: (425) 643-9954 E-mail: seabird@seabird.com Web: www.seabird.com

### **APPLICATION NOTE NO. 34**

# **Revised October 2012**

## Instructions for Use of Conductivity Cell Filling and Storage Device PN 50087 and 50087.1

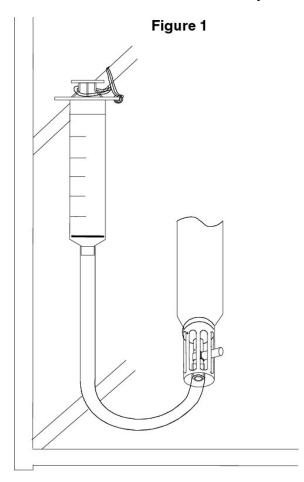



This application note provides instructions for use of PN 50087 / 50087.1 syringe and tubing assembly in rinsing, cleaning, and storing conductivity sensors. The tubing assembly consists of a length of 6.35 mm (1/4 inch) I.D. tube connected by a plastic reducing union to a short piece of 11.1 mm (7/16 inch) I.D. tube. Refer to *Application Note 2D: Instructions for Care and Cleaning of Conductivity Cells* for information on water and solutions recommended for use.

- SBE 9plus, 19plus V2, 25plus, and 49 are shipped with PN 50087.
- SBE 16plus V2 and 16plus-IM V2 are shipped with PN 50087.1, which includes the parts in 50087, plus hose barbs to replace the anti-foulant cap on the instrument. The hose barbs allow for connection of the tubing for cleaning and storing, as described below.

Note: This procedure can also be used with the SBE 16, 16*plus*, 16*plus*-IM, 19, 19*plus*, and 25, which are no longer in production.

#### **Procedure for Use**

- 1. To fill the conductivity cell, draw about 40-60 cc of solution into the syringe.
- 2. Connect the plastic tubing to the TC duct intake on the temperature sensor [Figure 1] (or to the open end of the conductivity cell on systems without the TC duct [Figure 2]), and inject solution into the cell and pump plumbing.
- CTDs with a TC duct or hose barb fitting remove the plastic reducing union and connect the smaller diameter tubing directly to the TC duct / fitting.
- CTDs without a TC duct or hose barb fitting (older instruments) leave the reducing union and large diameter tubing attached and carefully connect the tubing directly to the end of the glass conductivity cell [Figure 2].
- 3. (If applicable) Loop the rubber band around a bar on the CTD cage and back over the top of the syringe to secure the apparatus for storage.

# REMOVE THE SYRINGE AND TUBING ASSEMBLY BEFORE DEPLOYMENT!

# **Application Note Revision History**

Date	Description
1992	Initial release.
January 2005	Add reference to Application Note 2D for information on storing solutions.
	• Incorporate 50087.1 (kit with hose barbs for 16plus / 16plus-IM).
March 2008	Add applicability to V2 SeaCATs (16plus V2, 16plus-IM V2, 19plus V2)
October 2012	Update to include SBE 25plus.